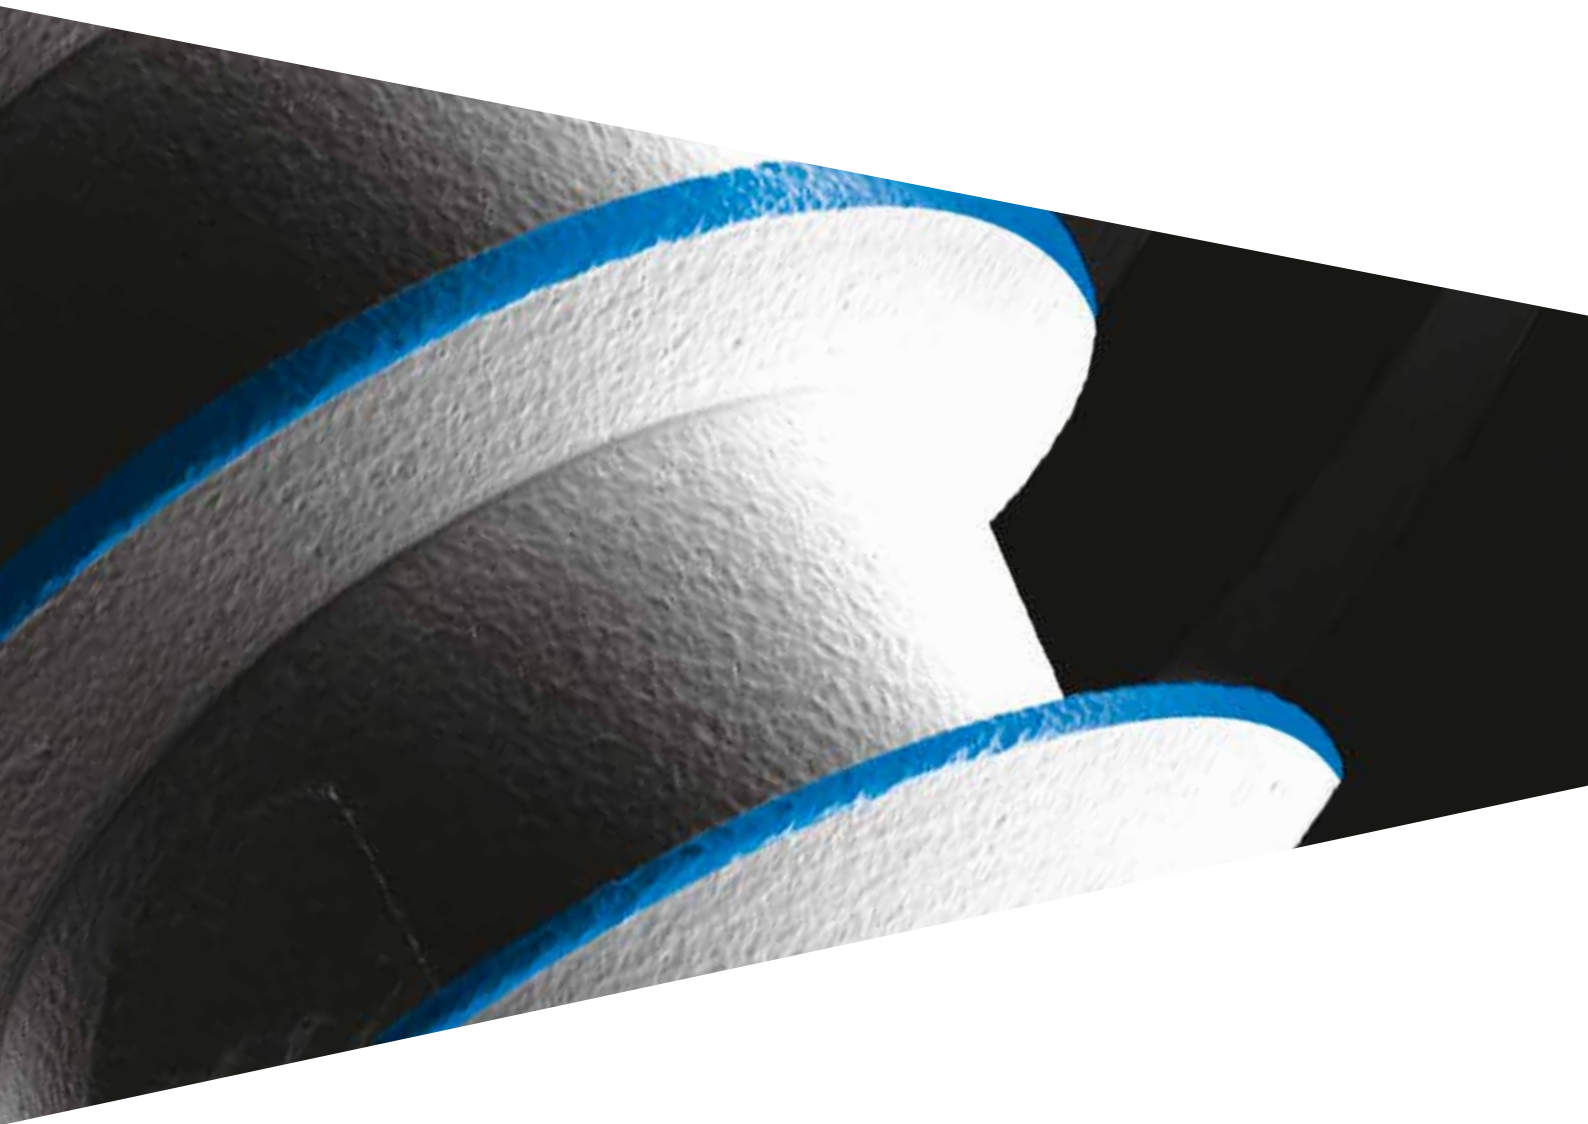


Product catalogue

SHELTA



Some products may not be regulatory cleared/released for sale in all markets.
Please contact the local Sweden & Martina or distributor sales office for current products availability.

Shelta

Table of contents



Implant system	4
Shelta implants	4
Shelta SL implants (Wide Thread)	5
Choosing the thread	6
ZirTi surface	7
Connection	8
Platform Switching	9
Mountless surgical procedure	10



The range	12
Shelta implants	12
Shelta SL implants (Wide Thread)	14



Surgical instruments	16
Surgical and prosthetic kit	16
Screw kit	18
Initial and intermediate drills	20
Final conical drills and stops	22
Parallelism pin, bone taps, and drills for distal sectors	24
Osteotomes	26
Additional instruments	28

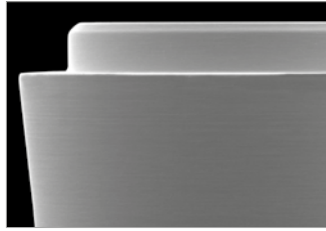


Prosthetic components	34
Healing abutments	34
Impression and model phase	36
SIMPLE temporary posts	40
Pre-made posts	42
Standard millable posts	46
Millable posts	48
B.O.P.T. prosthesis	50
Castable posts with base in alloy, titanium and cobalt chrome	52
Prosthesis on intermediate abutments	54
P.A.D. (Disparallel Screwed Prosthesis)	56
Straight P.A.D.	58
Angled P.A.D.	59
P.A.D. components for the relined and the cemented technique	63
P.A.D. prosthesis for "D.P.F." technique (Direct Prosthetic Framework)	64
Prosthesis on PLAIN abutments	66
T-Connect	68

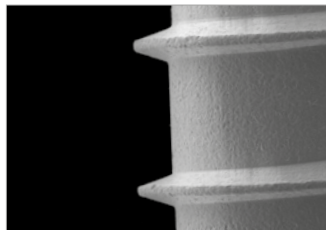


Overdenture	70
Locator abutment	70
Accessories for overdentures on Locator abutments	72
Overdentures anchored with ball attachments	74
Accessories for overdentures on ball attachments	76
Overdentures on bars	77
SFI-Bar	78

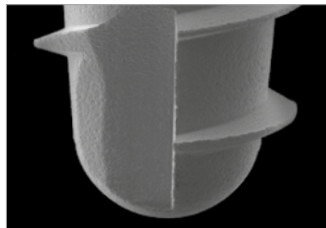
Shelta implants



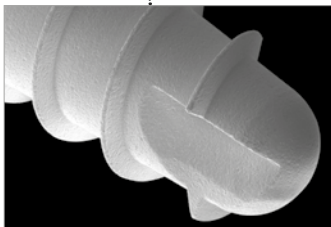
Shelta implants have a collar for prosthetic support and a machined neck.



The thread of Shelta implants is characterised by a triangular profile.



The thread of Shelta implants develops with the same geometry along the whole body of the implant.

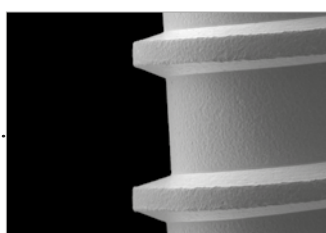


The apex of Shelta implants has two cut-outs that increase its penetration capacity and non-rotational property.

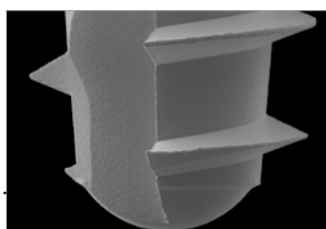
Shelta SL implants (Wide Thread)



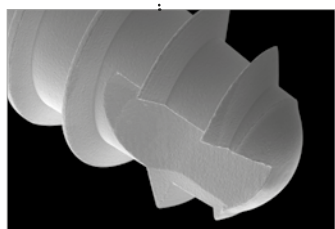
Shelta SL implants have the same prosthetic support collar and the same machined neck as Shelta implants.



The thread of Shelta SL implants maintains a constant pitch, but the depth varies along the implant body.



The thread of the Shelta implants maintains a constant outer thread diameter with a tapered inner body diameter. This results in pronounced and sharp apical threads.

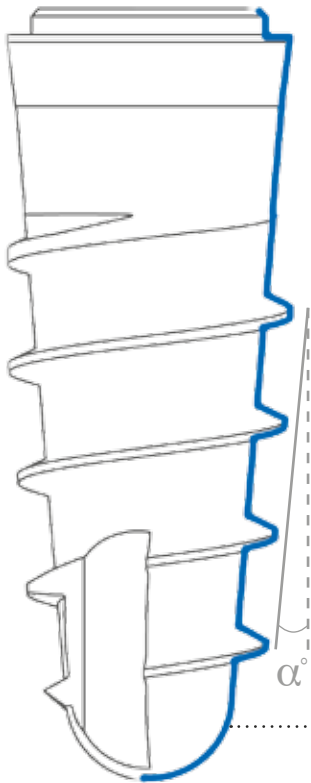


Shelta SL implants have a rounded apex, but the dimension is reduced due to the more pronounced threading.

Choosing the thread

Shelta and Shelta SL implants differ in the morphology of the apical part.

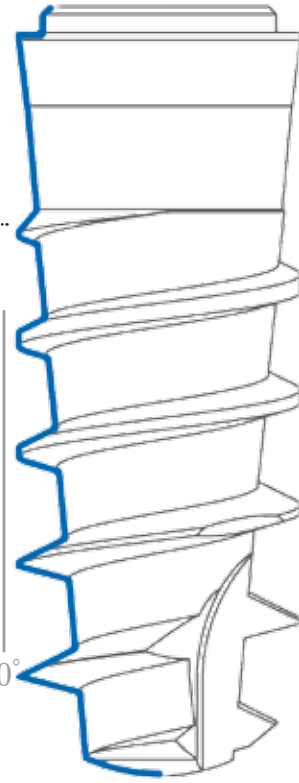
SHELTA



Shelta SL implants have a core with a conical geometric shape, though they maintain a constant cylindrical external diameter along the whole length of the implant. This characteristic means that the threading at the apex is much more accentuated.

In **Shelta** implants both the core of the implant and the threading have a conical morphology. Furthermore, unlike Shelta SL implants, the apex is a complete hemisphere with the presence of a less aggressive thread.

SHELTA SL



The crest of the thread of **Shelta SL** implants increases gradually in the coronal direction. This increases the high cutting capacity of the most apical threads.

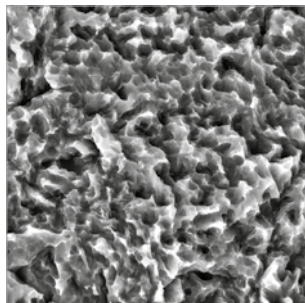
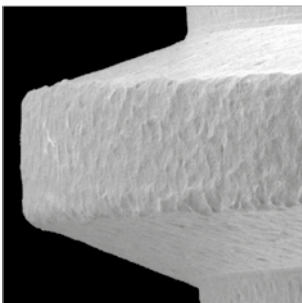
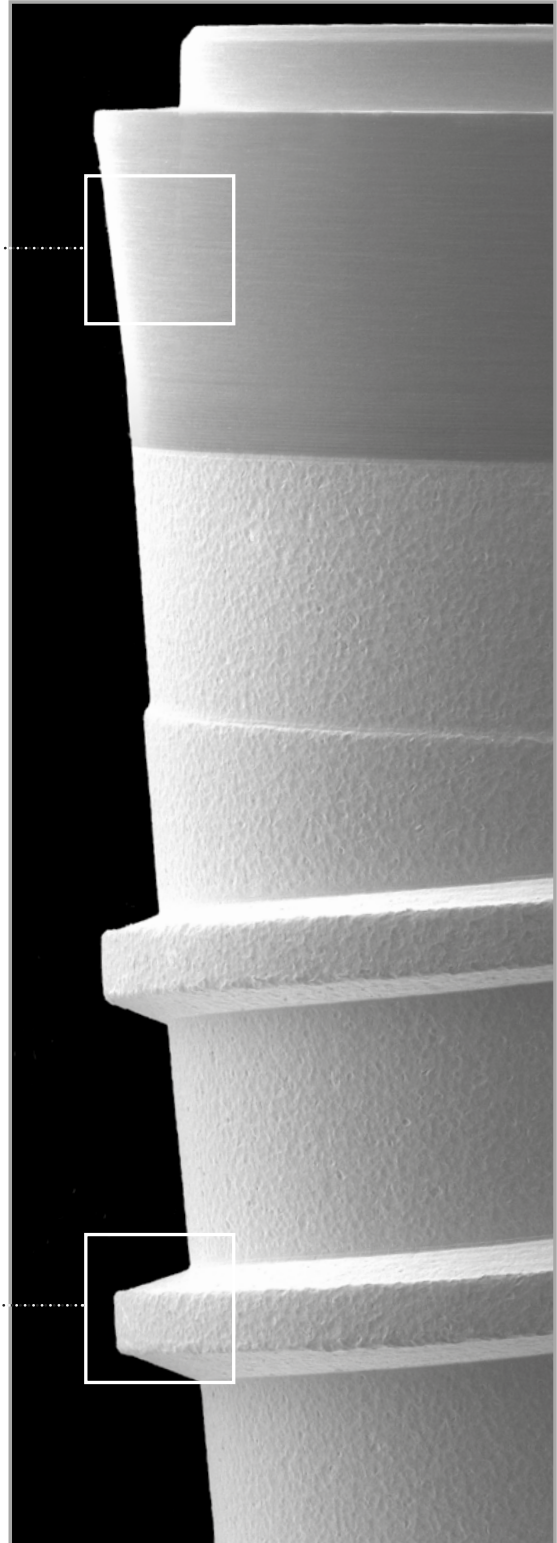
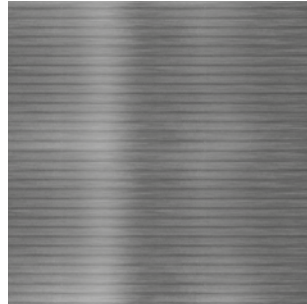
The crest of the thread of **Shelta** implants, on the other hand, is constant along the whole body of the fixture.



ZirTi surface

(Zirconium Sand-Blasted Acid Etched Titanium)

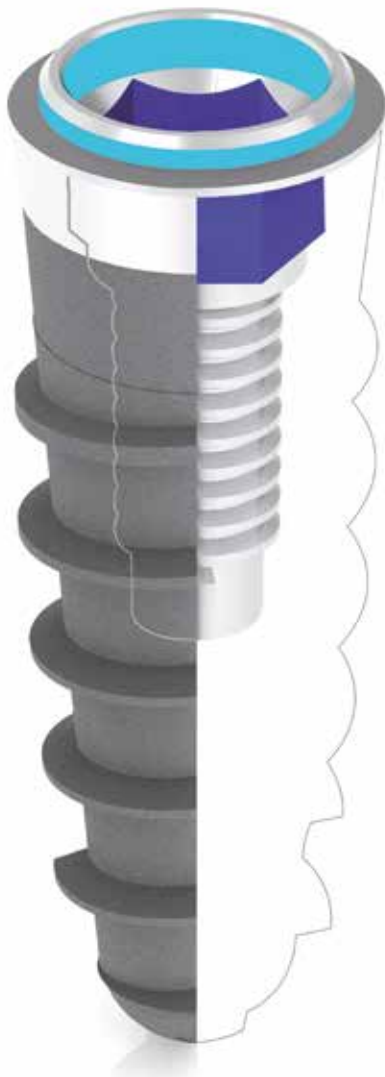
The **machined collar** prevents the accumulation of plaque in the area where the post joins the implant.



Shelta and Shelta SL implants are available in ZirTi surface. The implant body is treated with appropriate subtraction techniques that give the surface the characteristic ZirTi morphology.

Connection

Shelta and Shelta SL implants have a common prosthetic connection geometry, thus facilitating the task of the restoring doctor, independent of the implant platform diameter. This connection is the same as that of the \varnothing 3.80 mm implants in the Premium (and Premium SP) family by Sweden & Martina.



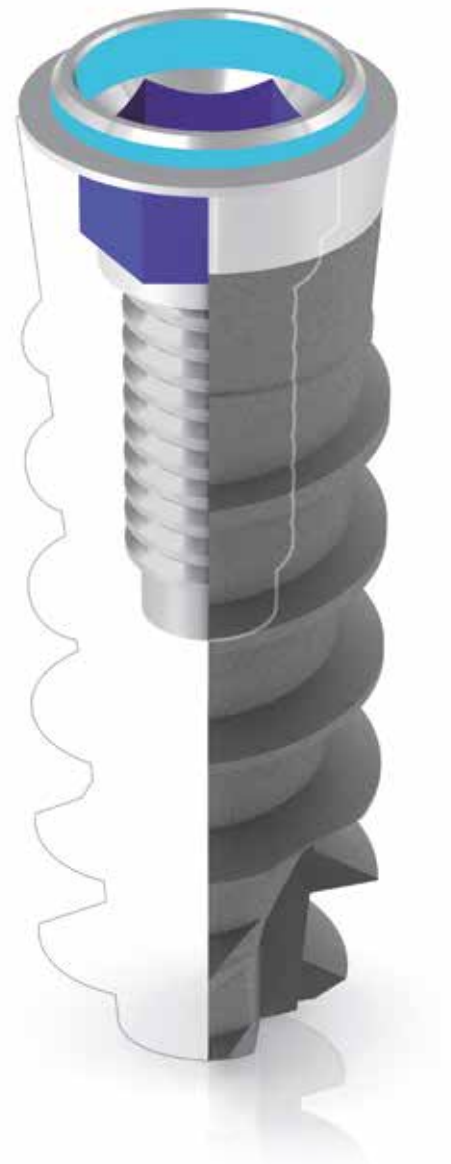
Collar

A collar is present on the top of the implant neck.

The internal part of the collar allows safe and easy engaging of the insertion drivers.

Internal hexagon for repositioning of the prosthesis

Located in a coronal position, it is characterised by good visibility.



Platform Switching

The Platform Switching is a prosthetic rehabilitation technique that aims to distance the prosthetic connection platform from the cervical bone.

All Shelta implants have a single connection hexagon, over which is a collar that is the same on all platforms: this considerably simplifies prosthesis management. The posts are available in two diameters, 3.30 mm and 3.80 mm.

Diameter 3.80 mm posts can be used with the Platform Switching technique on \varnothing 4.25 mm and \varnothing 5.00 mm implants, as shown in the pictures below.

\varnothing 3.80 post



\varnothing 3.80 implant

\varnothing 3.80 post



\varnothing 4.25 implant

\varnothing 3.80 post



\varnothing 5.00 implant

Platform Switching on Shelta implants \varnothing 3.80 mm

Should the prosthodontist wish to use the Platform Switching technique with the \varnothing 3.80 mm implant, this can be done using the \varnothing 3.30 mm posts of the Premium family by Sweden & Martina (see from page 42) as shown below.

\varnothing 3.30 post



\varnothing 3.80 implant



The standard \varnothing 3.30 mm posts perform prosthetic switching on \varnothing 3.80 implants resting on the external collar of the implants, and thus increasing the mismatching measurement.

Important warning

Considering the reduced diameter of \varnothing 3.30 mm prosthetic components, it is recommended to use them exclusively on \varnothing 3.80 mm implants for single crowns in front sectors (excluding premolars), and only as a support for multiple prostheses in distal sectors.

Mountless surgical procedure

The implant does not require a mounter for inserting into the implant site because it is engaged directly inside the connection by practical Easy Insert drivers designed to guarantee a safe grip.



A single instrument that allows the insertion of all Shelta implant diameters.

The **colour code** on the instrument shank and on the retaining metal O-rings facilitates the identification and choice of the item needed.

The Easy Insert drivers aid **visibility of the operating field**, do not occupy much space, and allow adjusting the connection hexagon properly because their hexagonal visual index is the same as a prosthetic index.

Engagement is obtained with a **titanium O-ring** that engages inside the connection.

Key to the implant codes

The implant codes are so-called “mnemonic” codes, i.e. they allow easy identification of the piece. Below is a table showing how the mnemonic codes work using code SH-ZT-380SL-115 as an example:

Type of implant	Surface	Diameter	Thread	Length
SH- SH: Shelta Implant	ZT- ZT: ZirTi surface	380 380: 3.80 mm 425: 4.25 mm 500: 5.00 mm	SL- SL: Wide Thread	115 085: 8.50 mm 100: 10.00 mm 115: 11.50 mm 130: 13.00 mm 150: 15.00 mm
		<i>is the size of the diameter of the implant platform</i>	<i>if no specifications are available, it refers to a standard thread (that is a thread that maintains its geometry along the body of the implant)</i>	<i>refers to the length of the implant</i>

All measurements in this catalogue are given in mm, unless indicated otherwise.

Table of colour codes

A colour code system has been defined in the Shelta implant system for identifying the intraosseous diameter of the implant.

The final drills and the sequence on the surgical tray are also identified with the colour code.

implant diameter	Ø 3.80	Ø 4.25	Ø 5.00
Colour code on the pack			

Important warning

The prosthetic components do not follow this colour code system, and should only be considered for the surgical phase.

Shelta implants

Shelta implants are characterised by a tapering that gradually decreases as the length of the implants increases. The angle remains unchanged between implants of different diameters, but of the same length.



implant diameter	Ø 3.80 mm	Ø 4.25 mm	Ø 5.00 mm
8.50	SH-ZT-380-085 	SH-ZT-425-085 	SH-ZT-500-085 
10.00	SH-ZT-380-100 	SH-ZT-425-100 	SH-ZT-500-100 
11.50	SH-ZT-380-115 	SH-ZT-425-115 	SH-ZT-500-115 
13.00	SH-ZT-380-130 	SH-ZT-425-130 	SH-ZT-500-130 
15.00	SH-ZT-380-150 	SH-ZT-425-150 	SH-ZT-500-150 
Surgical cover screws*	SH-VT-380 	SH-VT-380 	SH-VT-380 



















* Each implant is sold with its own surgical cover screw.

Recommened torque for surgical cover screw: 8-10 Ncm.

Shelta SL implants (Wide Thread)

The conical geometry of Shelta SL implants replicates that of Shelta implants with a standard thread with the same length and connection diameter.



implant diameter	Ø 3.80 mm	Ø 4.25 mm	Ø 5.00 mm
8.50	SH-ZT-380SL-085 	SH-ZT-425SL-085 	SH-ZT-500SL-085 
10.00	SH-ZT-380SL-100 	SH-ZT-425SL-100 	SH-ZT-500SL-100 
11.50	SH-ZT-380SL-115 	SH-ZT-425SL-115 	SH-ZT-500SL-115 
13.00	SH-ZT-380SL-130 	SH-ZT-425SL-130 	SH-ZT-500SL-130 
15.00	SH-ZT-380SL-150 	SH-ZT-425SL-150 	SH-ZT-500SL-150 
Surgical cover screws*	SH-VT-380 	SH-VT-380 	SH-VT-380 

* Each implant is sold with its own surgical cover screw.

Recommened torque for surgical cover screw: 8-10 Ncm.

Surgical kit

The instruments included in the Shelta surgical kit are made of steel for surgical use, have their descriptions screen-printed on the tray to allow the user to identify each instrument more easily and to put it back, with the aid of a colour code system that traces the suitable surgical procedures for the various implant diameters.




The Shelta surgical kit is also supplied with the templates for the graphic representation of the implant measurements to allow choosing the most suitable implant diameters and lengths by means of radiographic or tomographic analyses.

The surgical kit has very compact dimensions.



A torque-control ratchet is also included that acts as a torque-control ratchet for checking the closing torque of the prosthetic screws and as a surgical key for inserting the implants.

The kit consists of a box in Radel with a surgical tray inside that is set-up to hold the instruments according to a guided procedure. The sequences of use of the instruments are indicated by coloured marks.

description	code
Complete surgical kit of the instruments necessary for Shelta and Shelta SL implants	ZSHELTA-INT 
Kit with 5 spare silicon supports for surgical trays, for drills or instruments with right angle shanks	GROMMET-CA-1 
Kit with 5 spare silicon supports for surgical trays, for instruments fitted with connection hexagon	GROMMET-CA-2 




Screw kit

The Sweden & Martina Screw kit is a handy set containing the drivers necessary for the prosthetic phases, from the removal of the healing abutments to the final fastening of the over-structures, the drivers for standard abutments, straight profile P.A.D. and Locators and the drivers for ball attachments.

It includes digital and right angle drivers, a carrier for angled P.A.D. abutments and a torque-control ratchet.



Small and easy to carry, it allows simple and immediate management of the prosthetic rehabilitation phase after surgery.

description	code
Screw kit complete with prosthetic instruments	ZSCREW-INT 
Kit with 5 spare silicon supports for surgical trays, for drills or instruments with right-angle shanks	GROMMET-CA-1 
Kit with 5 spare silicon supports for surgical trays, for instruments fitted with connection hexagon	GROMMET-CA-2 

Initial and intermediate drills

All Sweden & Martina drills are made of steel for surgical use.

Precision drill: very sharp and precise, it facilitates the opening of the implant site.








Intermediate drill: has a shape with progressive diameter.

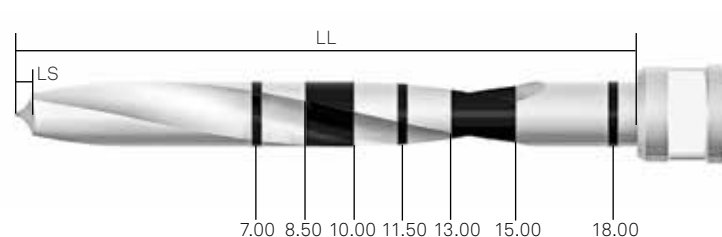


Pilot drill: presents different heights of the laser markings.

precision drill	intermediate drill	kit
<p>FS-230 precision drill</p> 	<p>FG-200/280XS intermediate drill, Ø 2.00 - 2.80 mm</p> 	<p>ZSHELTA-INT</p>

pilot drill and relative stops						kit
<p>FPT3-200-LXS pilot drill</p> 	<p>STOP3-200-085 8.50 mm pilot drill stop</p> 	<p>STOP3-200-100 10.00 mm pilot drill stop</p> 	<p>STOP3-200-115 11.50 mm pilot drill stop</p> 	<p>STOP3-200-130 13.00 mm pilot drill stop</p> 	<p>STOP3-200-150 15.00 mm pilot drill stop</p> 	<p>ZSHELTA-INT</p>

LL: Total length of the working part, including the tip.
LS: Length of the tip. This measurement must be calculated in addition to the length of the preparation hole.



Please note: The initial drills in this page and the conical drills shown on pages 22-23 always make a hole that is longer than the implant to be inserted. The oversizing (LS) is equal to the height of the tip of the drill that is being used. See drawing above.



















Final conical drills and stops

Also made of steel for surgical use, the final conical drills are characterised by four straight cutting edges.



Laser marking: the thickness of the laser marking corresponds to the height of the polished neck of the implants, thus allowing precise control of the depth of preparation of the surgical site.

Straight edge cut: the straight edge cut gives a great cutting capacity.

implant diameter	Ø 3.80 mm	Ø 4.25 mm	Ø 5.00 mm	kit
8.50	SH-FK380-085 	SH-FK425-085 	SH-FK500-085 	ZSHELTA-INT
10.00	SH-FK380-100 	SH-FK425-100 	SH-FK500-100 	ZSHELTA-INT
11.50	SH-FK380-115 	SH-FK425-115 	SH-FK500-115 	ZSHELTA-INT
13.00	SH-FK380-130 	SH-FK425-130 	SH-FK500-130 	ZSHELTA-INT
15.00	SH-FK380-150 	SH-FK425-150 	SH-FK500-150 	ZSHELTA-INT
stop	SH-STOP-FK380 	SH-STOP-FK425 	SH-STOP-FK500 	ZSHELTA-INT

LL: Total length of the working part, including the tip.
LS: Length of the tip. This measurement must be calculated in addition to the length of the preparation hole.



Please note: The drills always make a hole that is longer than the implant to be inserted. The oversizing (LS) is equal to the height of the tip of the drill that is being used (see drawing above).

Parallelism pin, bone taps, and drills for distal sectors

Shelta implants are self-tapping implants with excellent cutting and insertion capabilities. However, the use of a bone tap is recommended in all cases where the type of bone requires it. The absence of tapping in cases where this is recommended may lead to problems later when inserting the implant. As an option, shorter drills are available that are very practical in distal sectors with limited oral opening. They are available in the two diameters of cylindrical drills present in the surgical kit (\varnothing 2.00 and \varnothing 2.80 mm).



Bone taps: they are available both with right angle shank and with a connector for torque-control ratchet.

Distal drills: short length, for distal sectors with limited oral opening.

Parallelism pins: they have one side with \varnothing 2.00 mm and the other \varnothing 2.80 mm so as to be able to check the insertion axis of the implants from the preliminary hole with the \varnothing 2.00 mm drill length.

Parallelism pin

description	code	kit
Parallelism pin with one side \varnothing 2.00 and the other \varnothing 2.80 mm	PP-2/28	ZSHELTA-INT
Parallelism pin with depth marking, large version	PPTL-2-28	-
Parallelism pin with depth marking, small version	PPTS-2-28	-

Bone taps

description	\varnothing 3.80 mm	\varnothing 4.25 mm	\varnothing 5.00 mm	kit
Bone taps with right angle attachment	SH-MS-380-CA 	SH-MS-425-CA 	SH-MS-500-CA 	ZSHELTA-INT
Bone taps with hexagonal attachment	SH-MS-380 	SH-MS-425 	SH-MS-500 	-

Drills for distal sectors

description	code	kit
Cylindrical drill, \varnothing 2.00 mm	FPT5-200-LXS	-
Cylindrical drill, \varnothing 2.80 mm	FFT5-280-LXS	-

The parallelism pins with laser marking, the bone taps with hexagonal attachment and the drills for distal sectors are not included in any kit. They are to be ordered separately.

























Osteotomes

A set of osteotomes made of steel for surgical use is available, useful for maxillary sinus floor expansion and lift protocols via the crestal bone.

The laser-etched codes on the handles show the diameter of the osteotome, so as to facilitate recognition of the correct surgical sequence.



The use of osteotomes is ideal in bone expansion procedures.

implant diameter	Ø 3.80		Ø 4.25		Ø 5.00	
Osteotome for implant h. 8.50 mm and 10.00 mm	SH-OS-380-100-PP 	SH-OS-380-100-PR 	SH-OS-425-100-PP 	SH-OS-425-100-PR 	SH-OS-500-100-PP 	SH-OS-500-100-PR 
Osteotome for implant h. 11.50 mm	SH-OS-380-115-PP 	SH-OS-380-115-PR 	SH-OS-425-115-PP 	SH-OS-425-115-PR 	SH-OS-500-115-PP 	SH-OS-500-115-PR 
Osteotome for implant h. 13.00 mm	SH-OS-380-130-PP 	SH-OS-380-130-PR 	SH-OS-425-130-PP 	SH-OS-425-130-PR 	SH-OS-500-130-PP 	SH-OS-500-130-PR 
Osteotome for implant h. 15.00 mm	SH-OS-380-150-PP 	SH-OS-380-150-PR 	SH-OS-425-150-PP 	SH-OS-425-150-PR 	SH-OS-500-150-PP 	SH-OS-500-150-PR 
tip	flat	rounded	flat	rounded	flat	rounded

The osteotomes are not included in any kit. They are to be ordered separately.

Additional instruments




All the additional instruments for Shelta and Shelta SL implants, made of steel for surgical use, have been designed to offer maximum ergonomics and ease of use. All the instruments have a laser-marked code for easy identification of the pieces.





Easy Insert drivers: carrier and driver for implants.

Drivers: solid help for removing implants.




Carriers and drivers for implants

description	code	kit
Short driver with right angle shank	EASYC2-EX230-CA 	ZSHELTA-INT
Long driver with right angle shank	EASYL2-EX230-CA 	ZSHELTA-INT
Driver with connector for torque-control ratchet	EASY2-EX230-EX 	ZSHELTA-INT


Drivers

description	code	kit
Short driver (hex 2.30 mm)	BC-EX230 	ZSHELTA-INT
Long driver (hex 2.30 mm)	BL-EX230 	ZSHELTA-INT


Surgical screwdrivers

description	code	kit
Screwdriver for surgical cover screw and fixation screws, digital, extra-short	HSMXS-20-DG 	ZSHELTA-INT ZSCREW-INT
Screwdriver for surgical cover screw and fixation screws, digital, short	HSM-20-DG 	ZSHELTA-INT ZSCREW-INT
Screwdriver for surgical cover screw and fixation screws, digital, long	HSML-20-DG 	ZSHELTA-INT ZSCREW-INT










Torque-control ratchet

description	code	kit
Kit composed of a torque-control ratchet, which can be used in dynamometric or fixed mode, and accessories for quick torque adjustment and periodic maintenance. The ratchet has torque limits from 10 to 70 Ncm, with adjustment lines at 10-20-25-30-35-50-70 Ncm	CRI5-KIT 	ZSHELTA-INT ZSCREW-INT ZPA001E01







Prosthetic Accessories Kit

description	code
The Prosthetic Accessories Kit includes the torque-control ratchet, the long digital screwdriver with the connection for torque-control ratchet and the related hand knob. This kit is very useful for the prosthetic rehabilitation phase	ZPA001E01 


Prosthetic screwdrivers

description	code	kit
Screwdriver for fixation screws, with hexagonal connector for torque-control ratchet or hand knob, short	HSM-20-EX 	ZSHELTA-INT ZSCREW-INT
Screwdriver for fixation screws, with hexagonal connector for torque-control ratchet or hand knob, long	HSML-20-EX 	ZSHELTA-INT ZSCREW-INT ZPA001E01
Screwdriver for fixation screws, with hexagonal connector for torque-control ratchet or hand knob, extra-long	HSMXL-20-EX 	ZSCREW-INT
Screwdriver for fixation screws, with right angle shank	HSM-20-CA 	ZSHELTA-INT ZSCREW-INT
Screwdriver for ball attachments, with hexagonal connector for torque-control ratchet	BASCC-EX 	ZSCREW-INT
Screwdriver for straight P.A.D. abutments, with hexagonal connector for torque-control ratchet	AVV2-ABUT 	ZSCREW-INT
Driver for inserting Locator abutment, with hexagonal connector for torque-control ratchet, short	8926-SW 	ZSCREW-INT
Driver for inserting Locator abutment, with hexagonal connector for torque-control ratchet, long	8927-SW 	ZSCREW-INT
Instrument for assembly and maintaining the titanium cap for CAP-TIT-1 ball attachments	AVV-CAP-TIT-1 	ZSCREW-INT

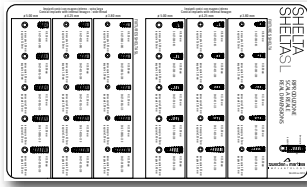
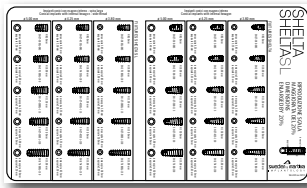
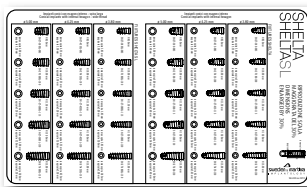
Extensions and adapters

description	code	kit
<p>Extension for bone taps, mounters, drivers and manual drivers, with hexagonal connector for torque-control ratchet</p>	<p>BPM-15</p> 	<p>ZSHELTA-INT ZSCREW-INT</p>
<p>Extension for surgical drills</p>	<p>PROF-CAL3</p> 	<p>ZSHELTA-INT ZSCREW-INT</p>
<p>Mechanical adapter with right angle shank for instruments with hexagonal connector</p>	<p>B-AVV-CA3</p> 	<p>ZSCREW-INT</p>
<p>Hand knob for instruments with hexagonal connection for torque-control ratchet</p>	<p>AVV3-MAN-DG</p> 	<p>ZSCREW-INT ZPA001E01</p>
<p>Knob for manual use of drivers, bone taps and drivers with contra-angle shank and with hexagonal connection for torque-control ratchet</p>	<p>AVV-CA-DG-EX</p> 	<p>ZSHELTA-INT</p>
<p>Carrier for transferring angled abutments into the oral cavity, sterilisable and reusable. It must be secured to the abutments with the screw PAD-VTRAL-140</p>	<p>PAD-CAR</p> 	<p>ZSCREW-INT</p>

Spare O-rings



description	code	kit
<p>Kit with 5 spare O-rings for all accessories with hexagonal connector for torque-control ratchet</p>	<p>ORING180-088</p> 	<p>-</p>

X-ray templates

description	code	kit
X-ray template for Shelta and Shelta SL implants, real dimensions	SH-L100 	ZSHELTA-INT
X-ray template for Shelta and Shelta SL implants, dimensions increased by 20%	SH-L120 	ZSHELTA-INT
X-ray template for Shelta and Shelta SL implants, dimensions increased by 30%	SH-L130 	ZSHELTA-INT

Bone profilers

The bone profilers are very useful for levelling a very irregular bone crest at the coronal level, especially in the subsequent use of P.A.D. abutments.

description	code
Bone profiler with narrow flaring	A-PAD-PS380-S 
Bone profiler with wide flaring	A-PAD-PS380-L 

The bone profilers are not included in any kit. They are to be ordered separately.

Healing abutments














The healing abutments in Gr. 5 titanium are identified by a laser-marking that reports the diameter, emergence profile and height. In case of healing abutments with straight emergence profile, the marking only reports the platform diameter and height. The healing abutments must be tightened at a torque of 10 Ncm, using the HSM series of drivers, the full details and codes of which can be found on 30-31.

The laser marking, shows the connection diameter (in the example 38 = 3.80 mm), the maximum crown size (in the example 46 = 4.60 mm) and the transgingival height (in the example 5 = 5.00 mm).



Guiding cylinder: facilitates centring when inserting the implant.

The laser marking, allows immediate recognition of the connection diameter (in the example 33 = 3.30 mm) and of the transgingival height (in the example 2 = 2.00 mm).

prosthetic component diameter	Ø 3.30 mm	Ø 3.80 mm
Healing abutments Anatomical emergence profile Transgingival height 2.00 mm	A-TMGR-330-2 	A-TMGR-380-2 
Healing abutments Anatomical emergence profile Transgingival height 3.00 mm	A-TMGR-330-3 	A-TMGR-380-3 
Healing abutments Anatomical emergence profile Transgingival height 5.00 mm	A-TMGR-330-5 	A-TMGR-380-5 
Healing abutments Anatomical emergence profile Transgingival height 7.00 mm	-	A-TMGR-380-7 
Healing abutments Straight emergence profile Transgingival height 2.00 mm	A-TMG-330-2 	A-TMG-380-2 
Healing abutments Straight emergence profile Transgingival height 3.00 mm	A-TMG-330-3 	A-TMG-380-3 
Healing abutments Straight emergence profile Transgingival height 5.00 mm	A-TMG-330-5 	A-TMG-380-5 

Important warning

The Ø 3.30 mm prosthetic components allow prosthetic Platform Switching with Ø 3.80 mm implants. It is recommended to use these posts exclusively for single crowns in front sectors (excluding premolars), and only as a support for multiple prostheses in distal sectors.

The Ø 3.80 mm prosthetic components are compatible with Ø 3.80 mm, Ø 4.25 mm and Ø 5.00 mm implants. They do not allow prosthetic Platform Switching on Ø 3.80 mm implants; they allow prosthetic Platform Switching on Ø 4.25 mm and Ø 5.00 mm implants.

Recommended torque for healing abutments: 8-10 Ncm.

Impression and model phase

The open tray and closed tray transfers are made of Gr. 5 titanium, anodised according to the colour code of the reference platform, facilitating the identification of any different diameters that may be used. The pull-up transfer is made of radiopaque PEEK to allow verification of the correct insertion in the implant platform.

Closed tray transfer: for taking impressions with the closed tray technique, the repositioning face allows the transfer to be put back in the impression material so as to reproduce the orientation of the connection precisely.


Open tray transfer: the retentive design provides a steady grip inside the impression.

Analog: anodised according to the colour code, like the transfers, to identify the different prosthetic platforms.






Pull-up transfer: the connection with tabs clicks into the implant connecting hexagon, without requiring a screw.

Analogs

prosthetic component diameter	Ø 3.30 mm	Ø 3.80 mm
Analogs	-	A-ANA-380 

Pull-up transfers







prosthetic component diameter	Ø 3.30 mm	Ø 3.80 mm
Pull-up transfers in radiopaque PEEK Straight emergence profile	A-TRAP-330 	-
Pull-up transfers in radiopaque PEEK Anatomical emergence profile	A-TRARP-330 	A-TRARP-380 

Important warning

The Ø 3.30 mm prosthetic components allow prosthetic Platform Switching with Ø 3.80 mm implants. It is recommended to use these posts exclusively for single crowns in front sectors (excluding premolars), and only as a support for multiple prostheses in distal sectors.





The Ø 3.80 mm prosthetic components are compatible with Ø 3.80 mm, Ø 4.25 mm and Ø 5.00 mm implants. They do not allow prosthetic Platform Switching on Ø 3.80 mm implants; they allow prosthetic Platform Switching on Ø 4.25 mm and Ø 5.00 mm implants.

Open tray transfers

prosthetic component diameter	Ø 3.30 mm	Ø 3.80 mm
<p>Open tray transfers Straight emergence profile Fixation screw included</p>	<p>A-TRA-330</p> 	<p>A-TRA-380</p> 
<p>Open tray transfers Anatomical emergence profile Fixation screw included</p>	<p>A-TRAR-330</p> 	<p>A-TRAR-380</p> 
<p>Single pack Fixation screws for open tray transfers Supplied with the transfers, it can also be ordered separately as a spare</p>	<p>VTRA2-180-15</p> 	<p>Use VTRA2-180-15</p>
<p>Single pack Fixation screws for open tray transfer, length 20.00, to be ordered separately as a spare</p>	<p>VTRA2-180-20</p> 	<p>Use VTRA2-180-20</p>

Recommended torque for transfer screws: 8-10 Ncm.

Closed tray transfers

prosthetic component diameter	Ø 3.30 mm	Ø 3.80 mm
Closed tray transfers Straight emergence profile Fixation screw included	<p>A-TRAS-330</p> 	-
Closed tray transfers Anatomical emergence profile Fixation screw included	<p>A-TRARS-330</p> 	<p>A-TRARS-380</p> 
Single pack Fixation screws for closed tray transfers Supplied with the transfers, it can also be ordered separately as a spare	<p>VTRA2-180-10</p> 	Use VTRA2-180-10

Important warning

The Ø 3.30 mm prosthetic components allow prosthetic Platform Switching with Ø 3.80 mm implants. It is recommended to use these posts exclusively for single crowns in front sectors (excluding premolars), and only as a support for multiple prostheses in distal sectors.

The Ø 3.80 mm prosthetic components are compatible with Ø 3.80 mm, Ø 4.25 mm and Ø 5.00 mm implants. They do not allow prosthetic Platform Switching on Ø 3.80 mm implants; they allow prosthetic Platform Switching on Ø 4.25 mm and Ø 5.00 mm implants.

Recommended torque for transfer screws: 8-10 Ncm.

SIMPLE temporary posts

The SIMPLE prosthetic protocol calls for creating temporary posts. They are made in Gr. 5 titanium or in PEEK with titanium base, and they are available in repositionable or non-repositionable version.

















PEEK posts with titanium base: for cemented-retained single crowns.

Aesthetic temporary posts without repositioning hexagon and with narrow transgingival profile for multiple temporary structures screwed directly onto the implants.

Temporary posts with hexagon for making simple screwed temporary posts.

The **hexagon** which provides the non-rotational aspect makes this post perfect for making single screwed temporary posts.

prosthetic component diameter	Ø 3.30 mm	Ø 3.80 mm
SIMPLE temporary posts in PEEK with a Gr. 5 titanium base Repositionable Straight emergence profile Fixation screw included	A-MPSC-330 	-
SIMPLE temporary posts in PEEK with a Gr. 5 titanium base Repositionable Anatomical emergence profile Fixation screw included	A-MPSCR-330 	A-MPSCR-380 
SIMPLE temporary posts in Gr. 5 titanium Repositionable Anatomical emergence profile Fixation screw included	A-MPSA-330-EX 	A-MPSA-380-EX 
SIMPLE temporary posts in Gr. 5 titanium Repositionable Straight emergence profile	A-MPSCI-330-EX 	A-MPSCI-380-EX 
SIMPLE temporary aesthetic posts in Gr. 5 titanium Non-repositionable Wide emergence profile Fixation screw included	A-MPSA-330 	A-MPSA-380 
SIMPLE temporary posts in Gr. 5 titanium Non-repositionable Straight emergence profile	A-MPSCI-330 	A-MPSCI-380 
SIMPLE temporary aesthetic posts in Gr. 5 titanium Non-repositionable Wide emergence profile Fixation screw included	A-MPS-330 	A-MPS-380 
Single pack Pack of 10 pieces Fixation screw for posts Supplied with the temporary posts, it can also be ordered separately as a spare	VM2-180 VM2-180-10 	Use VM2-180

Important warning

The Ø 3.30 mm prosthetic components allow prosthetic Platform Switching with Ø 3.80 mm implants. It is recommended to use these posts exclusively for single crowns in front sectors (excluding premolars), and only as a support for multiple prostheses in distal sectors.

The Ø 3.80 mm prosthetic components are compatible with Ø 3.80 mm, Ø 4.25 mm and Ø 5.00 mm implants. They do not allow prosthetic Platform Switching on Ø 3.80 mm implants; they allow prosthetic Platform Switching on Ø 4.25 mm and Ø 5.00 mm implants.

Recommended torque for fixation screws: 20-25 Ncm.

Pre-made posts

Made in Gr. 5 titanium, their colour is obtained through an oxidation process and, therefore, there is no type of coating, so it ensures the use of a highly biocompatible surface. The direct screw-retained posts have a well on the head into which is inserted the standard screwdriver of the system for inserting the posts (family HSM see pages 30-31 for the codes).

Angled posts: with a passing screw they offer 15° or 25° angles.

Colour: Their colour is suitable for prosthetic rehabilitations of particular aesthetic importance.





Solid one-piece abutment: they are useful for cementing multiple prostheses on parallel implants.

Hexagon: allows repositioning and the non-rotational aspect; this type of post is therefore indicated for making single structures.

prosthetic component diameter	Ø 3.30 mm	Ø 3.80 mm
Solid one-piece abutments Non-repositionable	A-MDAD-330 	A-MDAD-380 

Recommended torque: 25-30 Ncm.








prosthetic component diameter	Ø 3.30 mm	Ø 3.80 mm
Pre-made straight posts Repositionable Straight emergence profile Transgingival height 1.00 mm Fixation screw included	A-MD-330-1 	A-MD-380-1 
Pre-made straight posts Repositionable Straight emergence profile Transgingival height 2.00 mm Fixation screw included	A-MD-330-2 	A-MD-380-2 
Pre-made straight posts Repositionable Straight emergence profile Transgingival height 4.00 mm Fixation screw included	A-MD-330-4 	A-MD-380-4 
Single pack Pack of 10 pieces Fixation screw for posts Supplied with the posts, it can also be ordered separately as a spare	VM2-180 VM2-180-10 	Use VM2-180

Important warning






The Ø 3.30 mm prosthetic components allow prosthetic Platform Switching with Ø 3.80 mm implants. It is recommended to use these posts exclusively for single crowns in front sectors (excluding premolars), and only as a support for multiple prostheses in distal sectors.

The Ø 3.80 mm prosthetic components are compatible with Ø 3.80 mm, Ø 4.25 mm and Ø 5.00 mm implants. They do not allow prosthetic Platform Switching on Ø 3.80 mm implants; they allow prosthetic Platform Switching on Ø 4.25 mm and Ø 5.00 mm implants.

Recommended torque for fixation screws: 20-25 Ncm.

prosthetic component diameter	Ø 3.30 mm	Ø 3.80 mm
<p>Pre-made straight posts Repositionable Anatomical emergence profile Transgingival height 1.00 mm Fixation screw included</p>	<p>A-MDR-330-1</p> 	<p>A-MDR-380-1</p> 
<p>Pre-made straight posts Repositionable Anatomical emergence profile Transgingival height 2.00 mm Fixation screw included</p>	<p>A-MDR-330-2</p> 	<p>A-MDR-380-2</p> 
<p>Pre-made straight posts Repositionable Anatomical emergence profile Transgingival height 4.00 mm Fixation screw included</p>	<p>A-MDR-330-4</p> 	<p>A-MDR-380-4</p> 
<p>Single pack Pack of 10 pieces</p> <p>Fixation screw for posts Supplied with the posts, it can also be ordered separately as a spare</p>	<p>VM2-180 VM2-180-10</p> 	<p>Use VM2-180</p>

Recommended torque for fixation screws: 20-25 Ncm.

prosthetic component diameter	Ø 3.30 mm	Ø 3.80 mm
<p>Pre-made posts angled at 15° Repositionable Straight emergence profile Transgingival height 1.75 mm Fixation screw included</p>	<p>A-MA15-330</p> 	-
<p>Pre-made posts angled at 15° Repositionable Anatomical emergence profile Transgingival height 1.80 mm Fixation screw included</p>	<p>A-MAR15-330</p> 	<p>A-MAR15-380</p> 
<p>Pre-made posts angled at 25° Repositionable Anatomical emergence profile Transgingival height 1.80 mm Fixation screw included</p>	-	<p>A-MAR25-380</p> 
<p>Single pack Pack of 10 pieces</p> <p>Fixation screw for posts Supplied with the posts, it can also be ordered separately as a spare</p>	<p>VM2-180 VM2-180-10</p> 	<p>Use VM2-180</p>

Important warning

The Ø 3.30 mm prosthetic components allow prosthetic Platform Switching with Ø 3.80 mm implants. It is recommended to use these posts exclusively for single crowns in front sectors (excluding premolars), and only as a support for multiple prostheses in distal sectors.

The Ø 3.80 mm prosthetic components are compatible with Ø 3.80 mm, Ø 4.25 mm and Ø 5.00 mm implants. They do not allow prosthetic Platform Switching on Ø 3.80 mm implants; they allow prosthetic Platform Switching on Ø 4.25 mm and Ø 5.00 mm implants.

Recommended torque for fixation screws: 20-25 Ncm.

Standard millable posts









They are made of Gr. 5 titanium and are able to respond to complex anatomical requirements in terms of both narrow prosthetic spaces and parallel implants.

Pre-cut posts allow very pronounced angles to be reached, up to 25°, limiting the time needed to reduce them by milling.



Straight millable posts, with their profile in the shape of an inverted cone, are suitable for angles of up to 10° and small profiles.



prosthetic component diameter	Ø 3.30 mm	Ø 3.80 mm
Straight millable posts Repositionable Straight emergence profile Fixation screw included	A-MF-330 	A-MF-380 
Straight millable posts Repositionable Anatomical emergence profile Fixation screw included	A-MFR-330 	A-MFR-380 
Pre-cut millable posts Repositionable Straight emergence profile Fixation screw included	A-MFP-330 	-
Pre-cut millable posts Repositionable Anatomical emergence profile Fixation screw included	A-MFPR-330 	A-MFPR-380 
Single pack Pack of 10 pieces Fixation screw for posts Supplied with the temporary posts, it can also be ordered separately as a spare	VM2-180 VM2-180-10 	Use VM2-180

Important warning

The Ø 3.30 mm prosthetic components allow prosthetic Platform Switching with Ø 3.80 mm implants. It is recommended to use these posts exclusively for single crowns in front sectors (excluding premolars), and only as a support for multiple prostheses in distal sectors.

The Ø 3.80 mm prosthetic components are compatible with Ø 3.80 mm, Ø 4.25 mm and Ø 5.00 mm implants. They do not allow prosthetic Platform Switching on Ø 3.80 mm implants; they allow prosthetic Platform Switching on Ø 4.25 mm and Ø 5.00 mm implants.

Millable posts





The SIMPLE technique allows perfect conditioning of the mucosa starting with temporary posts (see pages 40-41) and uses a millable post with large dimensions for making a primarily custom-built final prosthesis.

Alternatively the Interceptiv Technique uses posts characterised by two wide faces, which guarantee unequivocal repositioning on a model developed from an impression taken directly on the posts.

The **millable posts** for the Interceptiv technique have an emergence profile that simplifies the taking of the impression with closed tray technique, while the two wide faces guarantee unequivocal repositioning.



SIMPLE millable posts have a very wide emergence profile which can be adapted to any anatomy which was obtained with SIMPLE temporary aesthetic posts in the immediate conditioning phase.

prosthetic component diameter	Ø 3.30 mm	Ø 3.80 mm
Millable posts for SIMPLE technique Repositionable Wide emergence profile Fixation screw included	A-MFS-330 	A-MFS-380 
Millable posts for interceptive technique Repositionable Fixation screw included	-	A-MFTI-380 
Single pack Pack of 10 pieces Fixation screw for posts Supplied with the posts, it can also be ordered separately as a spare	VM2-180 VM2-180-10 	Use VM2-180

Important warning

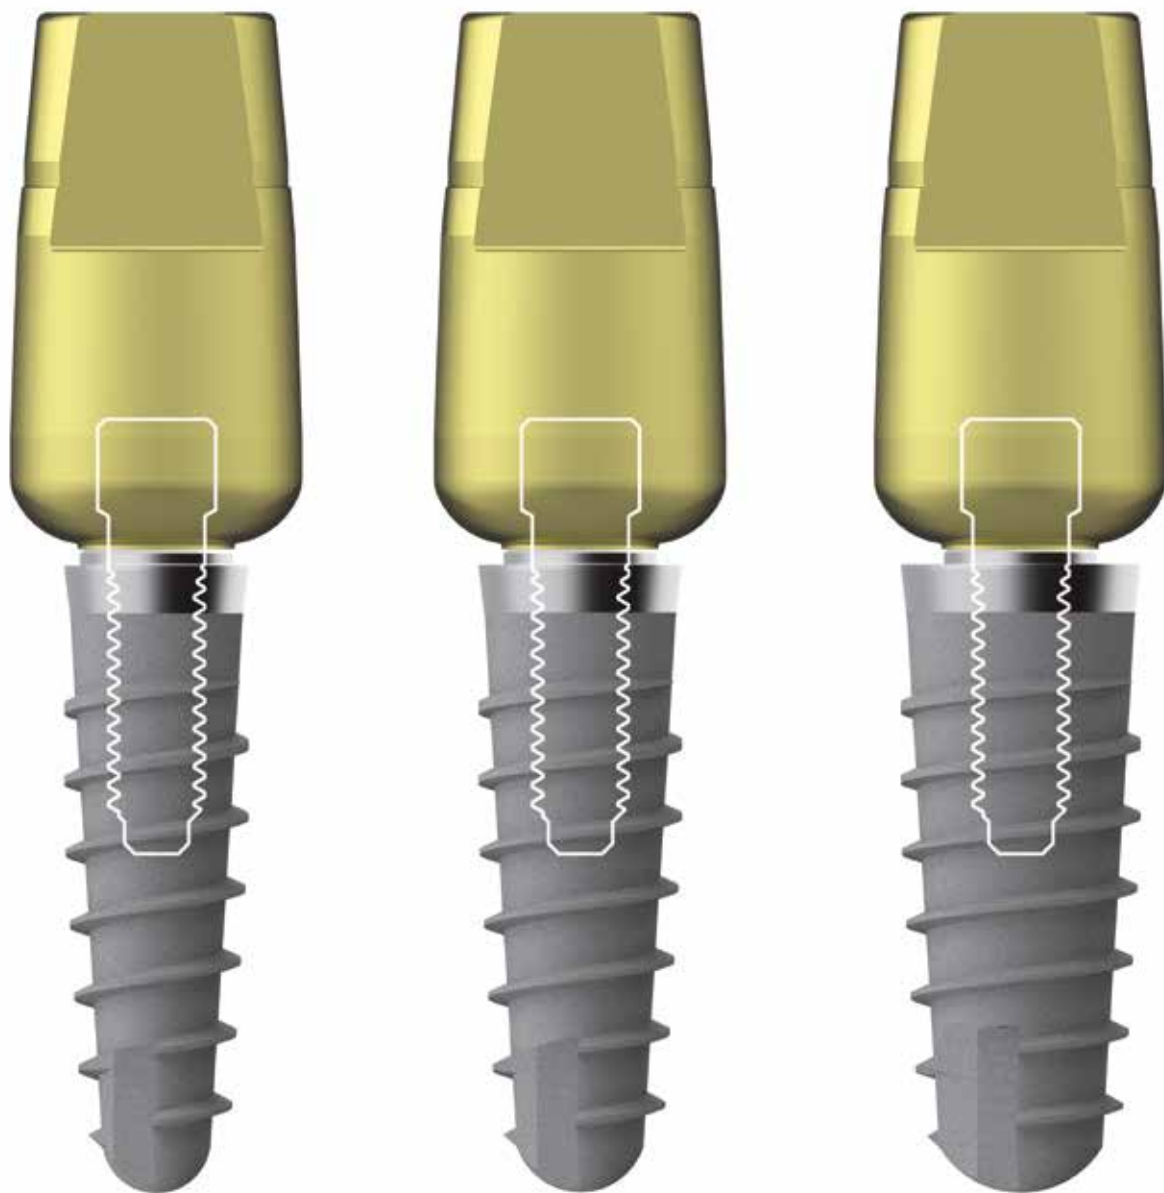
The Ø 3.30 mm prosthetic components allow prosthetic Platform Switching with Ø 3.80 mm implants. It is recommended to use these posts exclusively for single crowns in front sectors (excluding premolars), and only as a support for multiple prostheses in distal sectors.

The Ø 3.80 mm prosthetic components are compatible with Ø 3.80 mm, Ø 4.25 mm and Ø 5.00 mm implants. They do not allow prosthetic Platform Switching on Ø 3.80 mm implants; they allow prosthetic Platform Switching on Ø 4.25 mm and Ø 5.00 mm implants.

B.O.P.T. prosthesis

According to the principles of the B.O.P.T. technique (Biologically Oriented Preparation Technique) a simplified line has been developed that allows you to have only one post for all diameters of the Shelta line. This is possible thanks to the particular design of the connection, different from the classic connection, which allows it to rest safely on the platform of the centring collar.





The same B.O.P.T. millable post **A-MEFL-330** with a 2.30 mm hexagon is used on all diameters of Shelta implants, that is 3.80, 4.25 and 5.00 mm.



Shelta Ø 3.80

Shelta Ø 4.25

Shelta Ø 5.00

<p>for implants</p>	<p>Ø 3.80, 4.25, 5.00 mm</p>	
<p>B.O.P.T. healing abutment</p>	<p>A-TMG-MEFL-330</p>	
<p>B.O.P.T. millable post in titanium Fixation screw included</p>	<p>A-MEFL-330</p>	
<p>Pack of 5 pieces B.O.P.T. cap for taking the impression</p>	<p>CAP-MEFL-5</p> 	
<p>Single pack Pack of 10 pieces Fixation screws for B.O.P.T. posts Supplied with the posts, it can also be ordered separately as a spare</p>	<p>VM2-180 VM2-180-10</p> 	

Important warning













The B.O.P.T. prosthetic components are unique for all implants diameters, hex is 2.30 mm, the abutment rests on the external collar of the connection platform.

Recommended torque for fixation screws: 20-25 Ncm.

Castable posts with base in alloy, titanium and cobalt chrome

Castable posts with an alloy base combine the simplicity of castable solutions with a base of gold alloy, cobalt chrome or titanium, biocompatible materials. The melting point of the above-mentioned alloys is such as to preserve the base against dimensional alterations at the time of overcasting the castable part.



prosthetic component diameter	Ø 3.30 mm	Ø 3.80 mm
Castable posts with a pre-made base in gold alloy Repositionable Anatomical emergence profile Fixation screw included	A-UCR-330-EX 	A-UCR-380-EX 
Castable posts with a pre-made base in gold alloy Non-repositionable Anatomical emergence profile Fixation screw included	A-UCR-330 	A-UCR-380 
Castable posts with pre-made base in titanium Repositionable Anatomical emergence profile Fixation screw included	A-UCTR-330-EX 	A-UCTR-380-EX 
Castable posts with pre-made base in cobalt chrome Repositionable Anatomical emergence profile Fixation screw included	A-UCRCO-330-EX 	A-UCRCO-380-EX 
Castable posts with pre-made base in cobalt chrome Non-repositionable Anatomical emergence profile Fixation screw included	A-UCRCO-330 	A-UCRCO-380 
Spare castable sleeves for castable posts with alloy base Without fixation screw	A-CCUCR-330 	A-CCUCR-380 
Single pack Pack of 10 pieces Fixation screw for posts Supplied with the posts, it can also be ordered separately as a spare	VM2-180 VM2-180-10 	Use VM2-180

Important warning

The Ø 3.30 mm prosthetic components allow prosthetic Platform Switching with Ø 3.80 mm implants. It is recommended to use these posts exclusively for single crowns in front sectors (excluding premolars), and only as a support for multiple prostheses in distal sectors.

The Ø 3.80 mm prosthetic components are compatible with Ø 3.80 mm, Ø 4.25 mm and Ø 5.00 mm implants. They do not allow prosthetic Platform Switching on Ø 3.80 mm implants; they allow prosthetic Platform Switching on Ø 4.25 mm and Ø 5.00 mm implants.

Recommended torque for fixation screws: 20-25 Ncm.









Prosthesis on intermediate abutments

These abutments have a straight emergence profile and are made up of a repositionable Gr. 5 titanium base, characterised by a small upper cone with a height of 0.70 mm, the same for all the connection diameters, which allows insertion and removal of multiple over-structures. The abutment is supplied with a castable sleeve for modelling and casting the over-structure and with the passing screw.

Normally, when these abutments are used, the impression is taken directly on the implants using the transfers. When the titanium base of the abutments is used to make a temporary post, the impression is transferred to the laboratory with the use of the special transfers and the castable sleeve is sent to the laboratory with the relative fixation screw.

A titanium sleeve is normally used to create the temporary prosthesis, which is supplied complete with the relative fixation screw.



description	code
Straight abutments with fixation screw Repositionable Transgingival height 1.00 mm Fixation screw included	A-ABU-380-1 
Straight abutments with fixation screw Repositionable Transgingival height 2.00 mm Fixation screw included	A-ABU-380-2 
Fixation screw for abutments Supplied with the abutments, it can also be ordered separately as a spare	A-VABU-180 
Open tray transfer for non repositionable standard abutments Fixation screw included	A-TRABU-380 
Single pack Spare screw for abutment transfers Supplied with the transfers, it can also be ordered separately as a spare	A-VTRABU-180 
Analog for non repositionable standard abutments Fixation screw included	A-ANABU-380 
Single pack Sleeves in titanium for abutments Fixation screw included	A-CTABU-380-ROT 
Single pack Spare castable sleeves for abutments Fixation screw not included	A-CCABU-380-ROT 

Important warning

The Ø 3.80 mm prosthetic components are compatible with Ø 3.80 mm, Ø 4.25 mm and Ø 5.00 mm implants. They do not allow prosthetic Platform Switching on Ø 3.80 mm implants; they allow prosthetic Platform Switching on Ø 4.25 mm and Ø 5.00 mm implants.

Recommended torque for fixation screws: 20-25 Ncm.
 Recommended torque for transfer screws: 8-10 Ncm.

P.A.D. (Disparallel Screwed Prosthesis)

The P.A.D. components (Disparallel Screwed Prosthesis) was designed to facilitate the production of multiple screwed prostheses.

The P.A.D. angled abutments are the solutions for implants positioned in distal saddles.




P.A.D. abutments: these all have the same upper cone, angled at 15°, which facilitates the manoeuvres of inserting and removing multiple screwed prostheses.





The upper cone allows further repositioning of the prosthetic structure by 15° on each side, which in the case of angled P.A.D. abutments are added to the angle of 17° or 30° . This characteristic allows easy management of disparallelism of up to 45° on each side.






Straight P.A.D.

<p>prosthetic component diameter</p>	<p>Ø 3.80 mm</p>
<p>Straight P.A.D. abutments Direct screw-retained Transgingival height 1.50 mm</p>	<p>A-PAD-AD380-15</p> 
<p>Straight P.A.D. abutments Direct screw-retained Transgingival height 3.00 mm</p>	<p>A-PAD-AD380-30</p> 
<p>Straight P.A.D. abutments Direct screw-retained Transgingival height 4.00 mm</p>	<p>A-PAD-AD380-40</p> 

Please note: to transfer straight abutments into the oral cavity each package contains a practical plastic carrier (code AVV-ABUT-DG, not available separately).

Recommended torque: 25-30 Ncm.








Angled P.A.D.






<p>prosthetic component diameter</p>	<p>Ø 3.80 mm</p>
<p>P.A.D. abutment angled at 17° Transgingival height 3.00 mm Fixation screw included</p>	<p>A-PAD-AA380-173</p> 
<p>P.A.D. abutment angled at 17° Transgingival height 5.00 mm Fixation screw included</p>	<p>A-PAD-AA380-175</p> 
<p>P.A.D. abutment angled at 30° Transgingival height 3.00 mm Fixation screw included</p>	<p>A-PAD-AA380-303</p> 
<p>P.A.D. abutment angled at 30° Transgingival height 5.00 mm Fixation screw included</p>	<p>A-PAD-AA380-305</p> 
<p>Single pack Pack of 10 pieces</p> <p>Fixation screw for P.A.D. abutments Supplied with the P.A.D. abutments, it can also be ordered separately as a spare</p>	<p>PAD-VM-180 PAD-VM-180-10</p> 

Important warning






The Ø 3.80 mm prosthetic components are compatible with Ø 3.80 mm, Ø 4.25 mm and Ø 5.00 mm implants. They do not allow prosthetic Platform Switching on Ø 3.80 mm implants; they allow prosthetic Platform Switching on Ø 4.25 mm and Ø 5.00 mm implants.

Recommended torque: 25-30 Ncm.

description	code
<p>Protection caps for P.A.D. abutments in Gr. 5 titanium, to be used if the abutments remain screwed to the implant during the lab phase. Fixation screw included (code PAD-VP-140), available also as a spare, to be tightened at 8-10 Ncm</p>	<p>PAD-CG</p> 
<p>Single pack Pack of 10 pieces</p> <p>Spare screw for P.A.D. abutment prosthetic components. Supplied with all the components for making the over-structure and also available as a spare</p>	<p>PAD-VP-140 PAD-VP-140-10</p> 
<p>Protection caps for P.A.D. abutments in PEEK, to be used if the abutments remain screwed to the implant during the lab phase. Recommended torque: 8-10 Ncm</p>	<p>PAD-CGP</p> 
<p>Rotating caps in POM for direct impression taking on P.A.D. abutments</p>	<p>PAD-CAP</p> 
<p>Non-rotating caps in POM for direct impression taking on P.A.D. abutments, with hexagon</p>	<p>PAD-CAP-EX</p> 
<p>Open tray transfer in Gr. 5 titanium for P.A.D. abutments, rotating. Long transfer screw included (code PAD-VTRAL-140), suitable for open impression tray and available also as a spare</p>	<p>PAD-TRA</p> 
<p>Open tray transfer in Gr. 5 titanium for P.A.D. abutments, with hexagon, non-rotating. Long transfer screw included (code PAD-VTRAL-140), suitable for open impression tray and available also as a spare</p>	<p>PAD-TRA-EX</p> 





description	code
<p>Spare long screw for P.A.D. abutment transfer Supplied with the transfers, it can be ordered separately as a spare</p>	<p>PAD-VTRAL-140</p> 
<p>Spare screw for P.A.D. abutment transfer Supplied with the transfers, it can be ordered separately as a spare</p>	<p>PAD-VTRA-140</p> 
<p>Analog for P.A.D. abutment in Gr. 5 titanium</p>	<p>PAD-ANA</p> 
<p>Castable sleeves in PMMA for P.A.D. abutments, rotating. Fixation screw included Attention: The recommended tightening torque for all the over-structures obtained by casting to the abutments is 20-25 Ncm. However, before casting, care must be taken in the laboratory to ensure that the castable sleeves are not fastened to the models with a torque exceeding 8-10 Ncm, because polymers are not as resistant as metal</p>	<p>PAD-CC</p> 
<p>Castable sleeves in PMMA for P.A.D. abutments, with hexagon, non-rotating. Fixation screw included Attention: The recommended tightening torque for all the over-structures obtained by casting to the abutments is 20-25 Ncm. However, before casting, care must be taken in the laboratory to ensure that the castable sleeves are not fastened to the models with a torque exceeding 8-10 Ncm, because polymers are not as resistant as metal</p>	<p>PAD-CC-EX</p> 

Recommended torque for transfer screws: 8-10 Ncm.

description	code
<p>PEEK sleeves for P.A.D. abutments, rotating. They are specifically for creating a temporary prosthesis or in cases when it is necessary to reline an old prosthesis to be used as a temporary one. Fixation screw included</p>	<p>PAD-CP</p> 
<p>PEEK sleeves for P.A.D. abutments, with hexagon, non-rotating. They are specifically for creating a temporary prosthesis or in cases when it is necessary to reline an old prosthesis for using as a temporary one. Fixation screw included, available also as a spare</p>	<p>PAD-CP-EX</p> 
<p>Castable posts in PMMA with a pre-made base in gold alloy, rotating, not repositionable, for overcasting on P.A.D. abutments. Fixation screw included, to be tightened at 20-25 Ncm. The head of the screw never rests on the PMMA, but always on the alloy base. The castable sleeve is also available as a spare (code A-CCUCR-330)</p>	<p>PAD-UC</p> 
<p>Castable posts in PMMA with a pre-made base in cobalt chrome, rotating, non-repositionable, for overcasting on P.A.D. abutments. Fixation screw included, to be tightened at 20-25 Ncm. The head of the screw never rests on the PMMA, but always on the alloy base. The castable sleeve is also available as a spare (code A-CCUCR-330)</p>	<p>PAD-UCRCO</p> 
<p>Single pack Pack of 10 pieces</p> <p>Spare screw for P.A.D. abutment prosthetic components. Supplied with all the components for making the over-structure and also available as a spare</p>	<p>PAD-VP-140 PAD-VP-140-10</p> 

Recommended torque for fixation screws: 20-25 Ncm.

P.A.D. components for the relined and the cemented technique

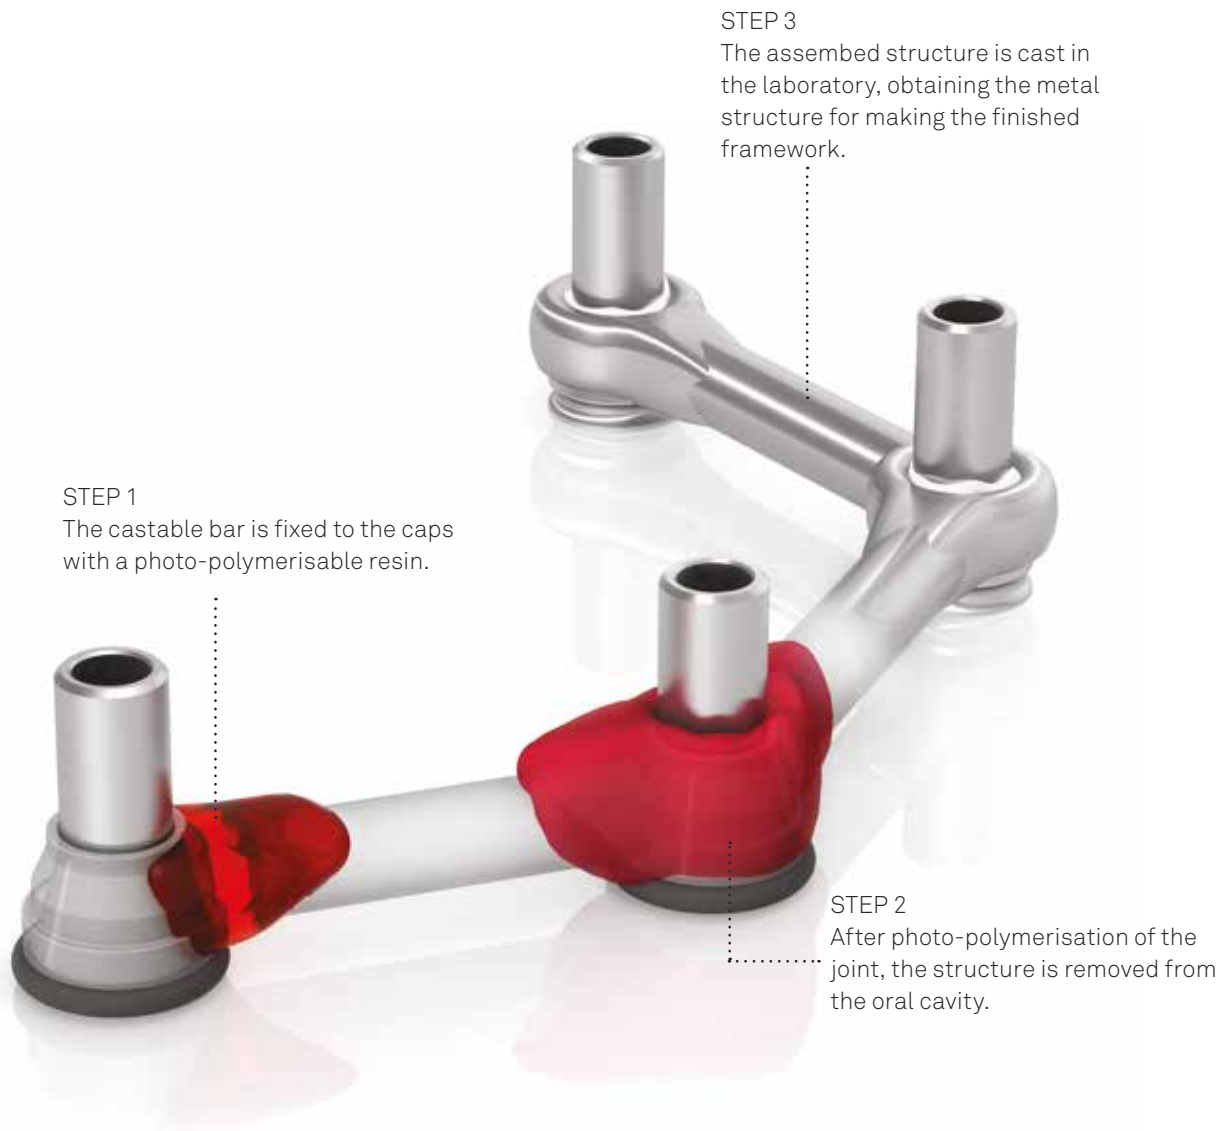
description	code
<p>Sleeves in Gr. 5 titanium for P.A.D. abutments, rotating. They are specifically for an immediate and final restoration process or for relining an old prosthesis to be used as a temporary post. Fixation screw included (code PAD-VP-140), available also as a spare</p>	<p>PAD-CT</p> 
<p>Sleeves in Gr. 5 titanium for P.A.D. abutments, with hexagon, non-rotating. They are specifically for an immediate and final restoration process or for relining an old prosthesis to be used as a temporary post. Fixation screw included (code PAD-VP-140), available also as a spare</p>	<p>PAD-CT-EX</p> 
<p>Castable posts in PMMA for cementing on titanium sleeves Effective for restoration without residual tensions</p>	<p>PAD-CCEM</p> 
<p>Single pack Pack of 10 pieces</p> <p>Spare screw for P.A.D. abutment prosthetic components Supplied with all the components for making the over-structure and also available as a spare</p>	<p>PAD-VP-140 PAD-VP-140-10</p> 








Recommended torque for fixation screws: 20-25 Ncm.

P.A.D. prosthesis for “D.P.F.” technique (Direct Prosthetic Framework)

The D.P.F. components have been specially developed for creating a castable resin structure directly in the oral cavity that is absolutely passive, not restricted by connection geometries due to the taking of the impression and the development of the model.

The temporary structure created with this technique can also be used as a positioning stent for making the final prosthesis.



description	code
<p>Set of all the prosthetic components for the “D.P.F.” technique on a single P.A.D. abutment. The set includes the titanium sleeve (PAD-CT-LV), the castable centring device (PAD-CC-LV), the anti-escape plug (PAD-TR-LV), the protective O-ring (PAD-ORING-LV) and the fixation screw (PAD-VP-140) to be tightened at 20-25 Ncm, available also as a spare</p>	<p>PAD-LV</p> 
<p>Spare titanium sleeve for the “D.P.F.” technique. The pack does not include the fixation screw</p>	<p>PAD-CT-LV</p> 
<p>Spare castable centring device for the “D.P.F.” technique</p>	<p>PAD-CC-LV</p> 
<p>Spare anti-escape plug for the “D.P.F.” technique</p>	<p>PAD-TR-LV</p> 
<p>Spare O-ring for the “D.P.F.” technique</p>	<p>PAD-ORING-LV</p> 
<p>Single pack Pack of 10 pieces</p> <p>Screw for P.A.D. abutment prosthetic components Supplied with all the components for making the framework and also available as a spare</p>	<p>PAD-VP-140 PAD-VP-140-10</p> 
<p>Castable bar, length 5.00 cm, Ø 2.20 mm</p>	<p>BARC</p> 

Recommended torque for fixation screws: 20-25 Ncm.

Prosthesis on PLAIN abutments










PLAIN abutments exploit the geometry of the upper part which, by means of a very small guide, is joined to normal castable sleeves.

The usefulness of these abutments is therefore that they allow centring and repositioning operations of structures screwed onto several implants.

The healing abutments allow optimum tissue conditioning thanks to an emergence profile that is flared at the crown. The healing caps do not have a passing screw but are inserted directly onto the abutment.



The PLAIN system also includes transfers and analogs in a single size, which allow the impression to be taken directly on the abutment. The open tray transfer has a long screw supplied with it.

prosthetic component diameter	Ø 3.80 mm	
PLAIN abutment Direct screw-retained Transgingival height 2.00 mm	A-PLAIN-ABU380-2	
PLAIN abutment Direct screw-retained Transgingival height 3.00 mm	A-PLAIN-ABU380-3	
PLAIN abutment Direct screw-retained Transgingival height 4.00 mm	A-PLAIN-ABU380-4	
Healing abutment for PLAIN abutment	A-PLAIN-CG380	
Castable sleeve for PLAIN abutments Fixation screw included	A-PLAIN-CC380	
Single pack Pack of 10 pieces Fixation screw for castable sleeve for PLAIN abutments. Supplied with the sleeves, it can also be ordered separately as a spare	A-PLAIN-VP200 A-PLAIN-VP200-10	
Analog for PLAIN abutment	A-PLAIN-ANA	
Transfer for PLAIN abutment Fixation screw included	A-PLAIN-TRA	
Spare screw for PLAIN transfer Supplied with the transfers for PLAIN abutments, it can also be ordered separately as a spare	A-PLAIN-VTRA200	

Important warning

The Ø 3.80 mm prosthetic components are compatible with Ø 3.80 mm, Ø 4.25 mm and Ø 5.00 mm implants. They do not allow prosthetic Platform Switching on Ø 3.80 mm implants; they allow prosthetic Platform Switching on Ø 4.25 mm and Ø 5.00 mm implants.




Please note: for transferring and tightening PLAIN abutments into the oral cavity, use the standard screwdrivers (code HSM-20-EX and HSML-20-EX for use with the torque-control ratchet) contained in the Shelta surgical kit.

Recommended torque for fixation screws: 20-25 Ncm.
Recommended torque for PLAIN abutments: 25-30 Ncm.
Recommended torque for transfer screws: 8-10 Ncm.

T-Connect

T-Connect supports can be used for making individualised posts in zirconium with open CAD CAM systems, with precision in the joint between the platforms that can be obtained with traditional components.



prosthetic component diameter	Ø 3.30 mm	Ø 3.80 mm
<p>T-Connect supports in Gr. 5 titanium height 4.00 mm for custom-made posts in zirconium Repositionable Fixation screw included</p>	<p>A-BASTZR-S-330-4</p> 	<p>A-BASTZR-S-380-4</p> 
<p>Single pack Pack of 10 pieces</p> <p>Spare screws for T-Connect supports Supplied with the T-Connect supports, it can also be ordered separately as a spare</p>	<p>VM2-180 VM2-180-10</p> 	<p>Use VM2-180</p>

Important warning

The Ø 3.30 mm prosthetic components allow prosthetic Platform Switching with Ø 3.80 mm implants. It is recommended to use these posts exclusively for single crowns in front sectors (excluding premolars), and only as a support for multiple prostheses in distal sectors.

The Ø 3.80 mm prosthetic components are compatible with Ø 3.80 mm, Ø 4.25 mm and Ø 5.00 mm implants. They do not allow prosthetic Platform Switching on Ø 3.80 mm implants; they allow prosthetic Platform Switching on Ø 4.25 mm and Ø 5.00 mm implants.

Recommended torque for fixation screws: 20-25 Ncm.










Locator abutment

Locator abutments* are a patented and versatile prosthetic solution for attaching overdentures to dental implants. The Locator system corrects misalignment of divergent implants up to 40° (20° for each implant) even in limited occlusal spaces. The abutments are made of Gr. 5 titanium and are available in different transgingival heights. Locator abutments use the special driver provided in the Screw kit and also available separately on request (code 8926-SW, short, and code 8927-SW, long).

See pages 72-73 for the list of accessories available.



* Locator abutments are medical devices manufactured and patented by Zest Anchors, Inc., 2061 Wineridge Place, Escondido, CA 92029, USA. Locator is a registered trademark of Zest Anchors, Inc. The European Agent for the purposes of MDD 93/42/EEC is Ventura Implant and Attachment Systems, 69 The Avenue, Ealing, London W13 8JR, England.












prosthetic component diameter	Ø 3.30 mm	Ø 3.80 mm
Locator Abutment Straight emergence profile Transgingival height 1.00 mm	1670 	1675 
Locator Abutment Straight emergence profile Transgingival height 2.00 mm	1671 	1676 
Locator Abutment Straight emergence profile Transgingival height 3.00 mm	1672 	1677 
Locator Abutment Straight emergence profile Transgingival height 4.00 mm	-	1678 
Locator Abutment Straight emergence profile Transgingival height 5.00 mm	-	1679 
Locator Abutment Straight emergence profile Transgingival height 6.00 mm	-	1680 











Important warning

The Ø 3.30 mm prosthetic components allow prosthetic Platform Switching with Ø 3.80 mm implants. It is recommended to use these posts exclusively for single crowns in front sectors (excluding premolars), and only as a support for multiple prostheses in distal sectors.

The Ø 3.80 mm prosthetic components are compatible with Ø 3.80 mm, Ø 4.25 mm and Ø 5.00 mm implants. They do not allow prosthetic Platform Switching on Ø 3.80 mm implants; they allow prosthetic Platform Switching on Ø 4.25 mm and Ø 5.00 mm implants.

Accessories for overdentures on Locator abutments

description	code
Kit containing 2 Gr. 5 titanium caps, 2 spacer rings in silicon rubber, 2 black processing polyethylene retainers (LDPE) with low retention capacity and 2 nylon retainers for each of the 4 different retention capacities	8519-2 
Kit containing 2 Gr. 5 titanium caps, 2 spacer rings in silicon rubber, 2 black processing polyethylene retainers (LDPE) with low retention capacity and 2 nylon retainers for each of the 4 different retention capacities, designed for severe disparallelism	8540-2 
Kit containing 2 steel caps, 2 spacer rings in silicon rubber, 2 black processing polyethylene retainers (LDPE) with low retention capacity and 2 nylon retainers for each of the 4 different retention capacities	8550-2 
Pack of 20 spacer rings in silicon rubber	8514 
Pack of 4 black processing polyethylene retainers (LDPE) with low retention capacity	8515 
Pack of 4 transparent nylon retainers, retention 5 lb	8524 
Pack of 4 pink nylon retainers, retention 3 lb	8527 
Pack of 4 blue nylon retainers, retention 1.5 lb	8529 
Pack of 4 green nylon retainers, retention 4 lb	8547 
Pack of 4 red nylon retainers, retention 1 lb	8548 
Pack of 4 orange nylon retainers, retention 2 lb	8915 

description	code
Pack of 4 aluminium analogs for Locator abutments, one size for all platforms	8530 
Pack of 4 aluminium transfers for Locator abutments, one size for all platforms. 4 black polyethylene retainers (LDPE) with low retention included (code 8515), available also as a spare	8505 
Pack of 4 black nylon parallelism pins (LDPE) for Locator abutments	8517 
Steel plate AISI 316L for measuring angles	9530 
Locator Core Tool. Steel instrument composed of a handle, driver (8390) for inserting Locator abutments, tip (8397) for inserting the retainers in the caps and the retention jacket (8394) for the driver (8390) for transferring the Locator abutments into the oral cavity	8393 
Replacement of the steel tip for inserting the retainers into the caps	8397 
Replacement of the steel driver for abutment screwing/unscrewing	8390 
Replacement of the retention jacket for the driver (8390) for transferring the Locator abutments into the oral cavity	8394 
Short driver in Gr. 5 titanium for torquing the Locator abutments. The driver is compatible with the torque-control ratchet	8926-SW 
Long driver in Gr. 5 titanium for torquing the Locator abutments. The driver is compatible with the torque-control ratchet	8927-SW 








* Locator abutments are medical devices manufactured and patented by Zest Anchors, Inc., 2061 Wineridge Place, Escondido, CA 92029, USA. Locator is a registered trademark of Zest Anchors, Inc. The European Agent for the purposes of MDD 93/42/EEC is Ventura Implant and Attachment Systems, 69 The Avenue, Ealing, London W13 8JR, England.


Overdentures anchored with ball attachments

There is a small hexagon at the base of the ball for attaching the driver. This driver is compatible with the system's torque-control ratchet.

See pages 76-77 for the list of the available matrices and respective accessories.



prosthetic component diameter	Ø 3.30 mm	Ø 3.80 mm
Ball attachments Straight emergence profile Transgingival height 1.00 mm	A-AS-330-1 	A-AS-380-1 
Ball attachments Straight emergence profile Transgingival height 2.00 mm	A-AS-330-2 	A-AS-380-2 
Ball attachments Straight emergence profile Transgingival height 4.00 mm	A-AS-330-4 	A-AS-380-4 
Analog of the ball attachment	ANAS 	Use ANAS

description	code
Steel driver for ball attachments, with connector for torque-control ratchet or digital connector Not included in the surgical kit, included in the Screw Kit and can be ordered separately	BASCC-EX 



Important warning

The Ø 3.30 mm prosthetic components allow prosthetic Platform Switching with Ø 3.80 mm implants. It is recommended to use these posts exclusively for single crowns in front sectors (excluding premolars), and only as a support for multiple prostheses in distal sectors.






The Ø 3.80 mm prosthetic components are compatible with Ø 3.80 mm, Ø 4.25 mm and Ø 5.00 mm implants. They do not allow prosthetic Platform Switching on Ø 3.80 mm implants; they allow prosthetic Platform Switching on Ø 4.25 mm and Ø 5.00 mm implants.

Accessories for overdentures on ball attachments


Polyamide caps for ball attachments

description	code
Polyamide cap for ball attachments Ø 2.20 mm	CAP-TFL-1 
Steel container for polyamide cap with outer Ø 4.80 mm The total height is 3.20 mm	CONT-CAP-TFL-1 





Titanium caps for ball attachments

description	code
Gr. 5 titanium cap complete with cap in two parts, titanium retention spring, and plastic mounting ring for ball attachments Ø 2.20 mm. The total height is 3.20 mm	CAP-TIT-1 
Spare plastic ring for titanium cap height 2.20 mm	AN-CAP-TIT-1 
Spare retention spring for titanium caps, average hardness, steel, Ø 3.20 mm	MOL1-CAP-TIT-1 
Spare retention spring for titanium cap, soft, for progressive adaptation of the prosthesis, steel, Ø 3.20 mm	MOL2-CAP-TIT-1 
Instrument for assembly and maintaining the titanium cap for CAP-TIT-1 ball attachments	AVV-CAP-TIT-1 

Caps in gold alloy for ball attachments





description	code
Cap in gold alloy, complete with plastic positioning ring for ball attachments Ø 2.20 mm. The total height is 3.10 mm, and the outside diameter is 3.50 mm	CAP-1 

O-ring retention devices for ball attachments

description	code	
Pack of 6 pieces Metal container in the shape of a ring for rubber O-rings. For ball attachments \varnothing 2.20 mm. The total height is 1.50 mm, and the outside diameter is 4.50 mm	99-440044*	
Pack of 12 pieces Red ring in silicon for laboratory use, outside \varnothing 4.50 mm, height 1.50 mm	99-443034*	
Pack of 12 pieces White ring in natural rubber, soft, outside \varnothing 4.50 mm, height 1.50 mm	99-443035*	
Pack of 12 pieces Black ring in natural rubber, hard, outside \varnothing 4.50 mm, height 1.50 mm	99-443036*	

* The retention O-rings for ball attachments are manufactured by Implant Direct Sybron International, 3050 East Hillcrest Drive, Thousand Oaks, CA 91362 U.S.A.
The European Agent for the purposes of MDD 93/42/EEC is Kerr Italia S.r.l., via Passanti 332, 84018 Scafati (SA) Italy.

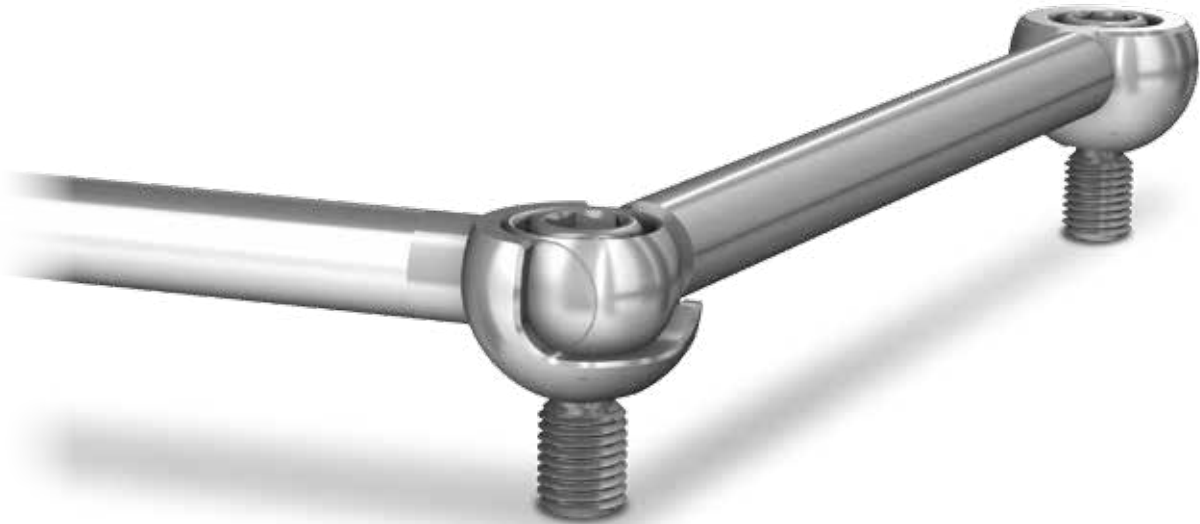
Overdentures on bars

description	code	
Castable bar, length 5.00 cm, height 3.00 mm, thickness 1.90 mm Ovoid-shaped profile with spacer	BARC-CAV-TIT	
Divisible bar attachment in titanium for oval bars with \varnothing 1.90 mm and height 3.00 mm	CAV-TIT	
Castable bar, length 5.00 cm, \varnothing 1.90 mm	BARC	
Bar attachment in gold alloy, for round bars with \varnothing 1.90 mm	CAV-375	




SFI-Bar*

SFI-Bar can be processed either chair-side or in the laboratory. The bar prostheses made with the SFI-Bar can be supported by 3, 4, 5 or 6 implants.

In case of repair it is possible to easily replace the individual elements.



* The components for SFI-Bar prostheses are medical devices manufactured by Cendres+Métaux, Rue de Boujean
122 CH-2501 Biel/Bienne.















prosthetic component diameter	Ø 3.30 mm	Ø 3.80 mm
Abutments for SFI-Bar Transgingival height 3.00 mm	-	05001001 
Abutments for SFI-Bar Transgingival height 4.00 mm	-	05001002 
Abutments for SFI-Bar Transgingival height 5.00 mm	-	05001003 


Important warning

The Ø 3.30 mm prosthetic components allow prosthetic Platform Switching with Ø 3.80 mm implants. It is recommended to use these posts exclusively for single crowns in front sectors (excluding premolars), and only as a support for multiple prostheses in distal sectors.

The Ø 3.80 mm prosthetic components are compatible with Ø 3.80 mm, Ø 4.25 mm and Ø 5.00 mm implants. They do not allow prosthetic Platform Switching on Ø 3.80 mm implants; they allow prosthetic Platform Switching on Ø 4.25 mm and Ø 5.00 mm implants.

OVERDENTURE

description	code	
2-implant kit, including: 2 large ball joint, 2 fixation screws, 1 tube bar in Gr. 5 titanium	05000337	
4-Implant kit, including: 2 large ball joint, 2 small ball joint, 2 Half shell balls, 4 fixation screws, 3 tube bars in Gr. 5 titanium	05000338	
Add-on kit, including: 1 small ball joint, 1 half shell ball, 1 fixation screw, 1 tube bar in Gr. 5 titanium	05000668	
Tube bar, length 20 mm, in Gr. 5 titanium	05000382	
Large ball joint in Gr. 5 titanium	05000383	
Small ball joint in Gr. 5 titanium	05000384	
Half shell ball in Gr. 5 titanium	05000385	
Fixation screw in Gr. 5 titanium	05000386	
Pack of 1 piece Female part asymmetrical, length 30.00 mm in gold alloy	05000344	
Female part complete, length 47.50 mm, in Gr. 5 titanium and plastic material. 1 bar with 12 segments, 6 yellow sheaths and 6 red sheaths	05000358	
Female part housing, length 47.50 mm in Gr. 5 titanium. 1 bar with 12 segments	05000387	
Pack of 6 pieces Yellow retention insert - smooth friction, in POM copolymer	05000388	
Pack of 6 pieces Red retention insert - normal friction, in POM copolymer	05000389	
Pack of 6 pieces Green retention insert - strong friction, in POM copolymer	05000390	

description	code
Instrument set	07000108 
Spacer Brass, ensures vertical resilience. Mount between female part and bar during polymerization	052082
Transfer jig length 26.00 mm	07000107
Tube bar gauge	07000106
Gauge aid	07000100
Screwdriver	07000114
Hex key	07000115
Thomas spanner key	070221
Insert positioner	07000036
Activator set	070198
Desactivator macro	070201
Tweezers	070347
Implant planner	07000111
Premium disk No. 1	08000101



rev. 01-16



Sweden & Martina S.p.A.

Via Veneto, 10
35020 Due Carrare (PD), Italy
Tel. +39.049.9124300
Fax +39.049.9124290
info@sweden-martina.com
www.sweden-martina.com

Sweden & Martina Mediterranea S.L.

Sorolla Center, Oficina 801
Avda Cortes Valencianas 58, 8pl
46015-Valencia, Spain
Tel. +34.96.3525895
Tel. 900993963
info.es@sweden-martina.com

Sweden & Martina Deutschland GmbH

Rupert-Mayer-Straße 46
D - 81379 München
Germany
Hotline 08001827699
info.de@sweden-martina.com

Sweden & Martina Inc.

c/o DCI Management
301 Pleasant St.
Abbottstown, 17301 PA, US
Toll free 844-8MARTINA
844-862-7846
info.us@sweden-martina.com

The implants, standard prosthetic components and surgical instruments contained in this catalogue are Medical Devices and are manufactured by Sweden & Martina S.p.A. They conform to the ISO 9001 and ISO 13485 standards and are certified with the CE Mark (Class I) and CE 0476 mark (Class IIA and class IIB) in compliance with European Medical Device Directive No. 93/42 and European Directive No. 2007/47/CE. They are conform to the QSR 21 CFR part 820 and are approved by FDA.

We have met the good manufacturing standards (GMP) set forth by many countries worldwide, including the United States FDA.



All trademarks herein are the property of Sweden & Martina S.p.A. unless otherwise indicated.
This material is intended for laboratories and clinicians and is not intended for patient distribution.
This material is not to be redistributed, duplicated, or disclosed without the express written consent of Sweden & Martina S.p.A.
For additional product information, including indications, contraindications, warnings, precautions, and potential adverse effects, see Sweden & Martina S.p.A. website.

The contents are updated at the time of publication. Check with the company for any subsequent updates.